

# AEC-NASA TECH BRIEF



AEC-NASA Tech Briefs announce new technology derived from the research and development program of the U.S. AEC or from AEC-NASA interagency efforts. They are issued to encourage commercial application. Tech Briefs are available on a subscription basis from the Clearinghouse for Federal Scientific and Technical Information, Springfield, Virginia 22151. Requests for individual copies or questions relating to the Tech Brief program may be directed to the Technology Utilization Division, NASA, Code UT, Washington, D.C. 20546.

## Neutron-Image Intensifier

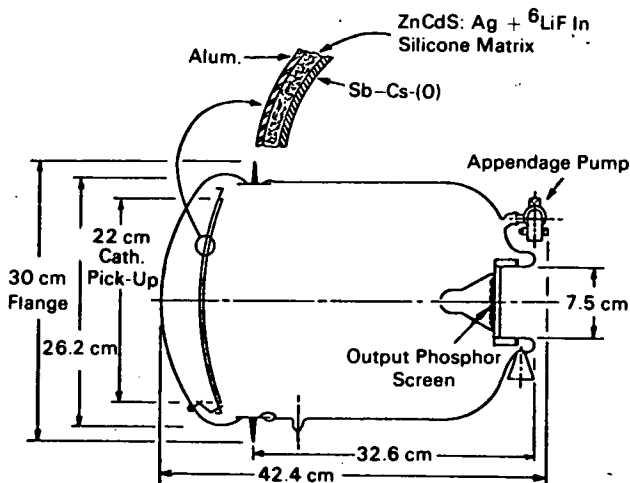


Diagram of a neutron-image intensifier tube; the expanded view shows a cross section of the neutron scintillator photoemissive target inside the tube.

### The problem:

To enhance the usefulness of neutron-radiographic techniques by providing prompt display of neutron images.

### The solution:

A neutron-image-intensification technique using a thermal-image intensifier tube similar to those used for detection of x-radiation. The tube, which detects and intensifies the pictorial image formed by neutrons, has a demagnification ratio of 9:1. The electronic intensifier tube comes in two sizes: one has a neutron-detection diameter of 22 cm; the other, 15 cm. In either case, a useful television signal can be obtained by optical coupling of a small-output phosphor-light image to a television camera.

### How it's done:

The radiation beam is directed toward the evacuated intensifier tube, as shown in the figure, in which it is converted into light by a phosphor or scintillator layer. The emitted light causes photoelectron-emission from an adjacent photoemissive layer. These electrons are voltage accelerated toward a phosphor output screen where a small, bright, visible signal is obtained. The image is intensified in the tube by the acceleration of the electron image and by the minification of that electron signal.

The neutron scintillator is a mixture of  $^6\text{LiF}$  and phosphor powders in a resin binder; the  $\text{LiF}$  contains 95.72%  $^6\text{Li}$ . The optimum mixture for light yield is 1 part  $^6\text{LiF}$  to 4 parts phosphor by weight. Two different phosphors,  $\text{ZnCdS}(\text{Ag})$  and  $\text{ZnS}(\text{Ag})$ , have been used in the scintillator. The latter is preferred because (1) its emission spectrum provides a good match for the spectral response of the adjacent photoemitter surface,  $\text{Sb-Cs}(0)$ ; and (2) its lower density yields less absorption for gamma radiation, thereby resulting in an improved neutron-gamma response ratio for the intensifier tube.

The detection mechanism with either phosphor is the same. The thermal neutrons are absorbed by the  $^6\text{Li}$ ; an alpha particle and a triton are promptly emitted. Each particle stimulates emission of light from the phosphor. A typical scintillator-target thickness of 0.4 mm absorbs about 30% of an incident thermal-neutron beam.

The light yield from a 15-cm-diameter neutron-intensifier tube provides linear response to thermal neutrons over at least four orders of neutron intensity. The excellent light-yield characteristics of the intensifier tube have permitted the observation of gross

(continued overleaf)

brightening of the output phosphor for incident thermal-neutron intensities as low as 100 neutrons per square centimeter-second for direct visual observation of the output-phosphor screen by dark-adapted observers. For television response, a vidicon television camera has provided similar gross images for incident thermal-neutron intensities as low as  $2 \times 10^4$  neutrons per square centimeter-second; an image orthicon television system has improved light-level response by a factor of 100 over the vidicon system.

Applications of the neutron-image intensifier include dynamic neutron-image studies involving heated, irradiated, reactor-fuel materials; water-flow and bubble-pattern studies in heat-transfer systems; and casting of heavy metals. Stationary images also can be observed with excellent sensitivity and speed. The tube may be useful as a detector for neutron-diffraction patterns also.

#### Reference:

Berger, H.: Neutron Image Intensifier. In Encyclopedic Dictionary of Physics, J. Thewlis, ed. Pergamon Press, in press.

#### Notes:

1. Neutron radiographers may be interested.
2. Inquiries concerning this innovation may be directed to:

Office of Industrial Cooperation  
Argonne National Laboratory  
9700 South Cass Avenue  
Argonne, Illinois 60439  
Reference: B70-10240

Source: H. Berger  
Metallurgy Division  
(ARG-10249)

#### Patent status:

Inquiries concerning rights for commercial use of this innovation may be made to:

Mr. George H. Lee, Chief  
Chicago Patent Group  
U.S. Atomic Energy Commission  
Chicago Operations Office  
9800 South Cass Avenue  
Argonne, Illinois 60439